


Printing the CVP Blood Report for ONLY QC Normal Control in Open Tube Mode

During your Daily QC runs or During your QC parallel study. **Print the CVP report exclusively for the Normal QC control!**
(Follow instructions below).

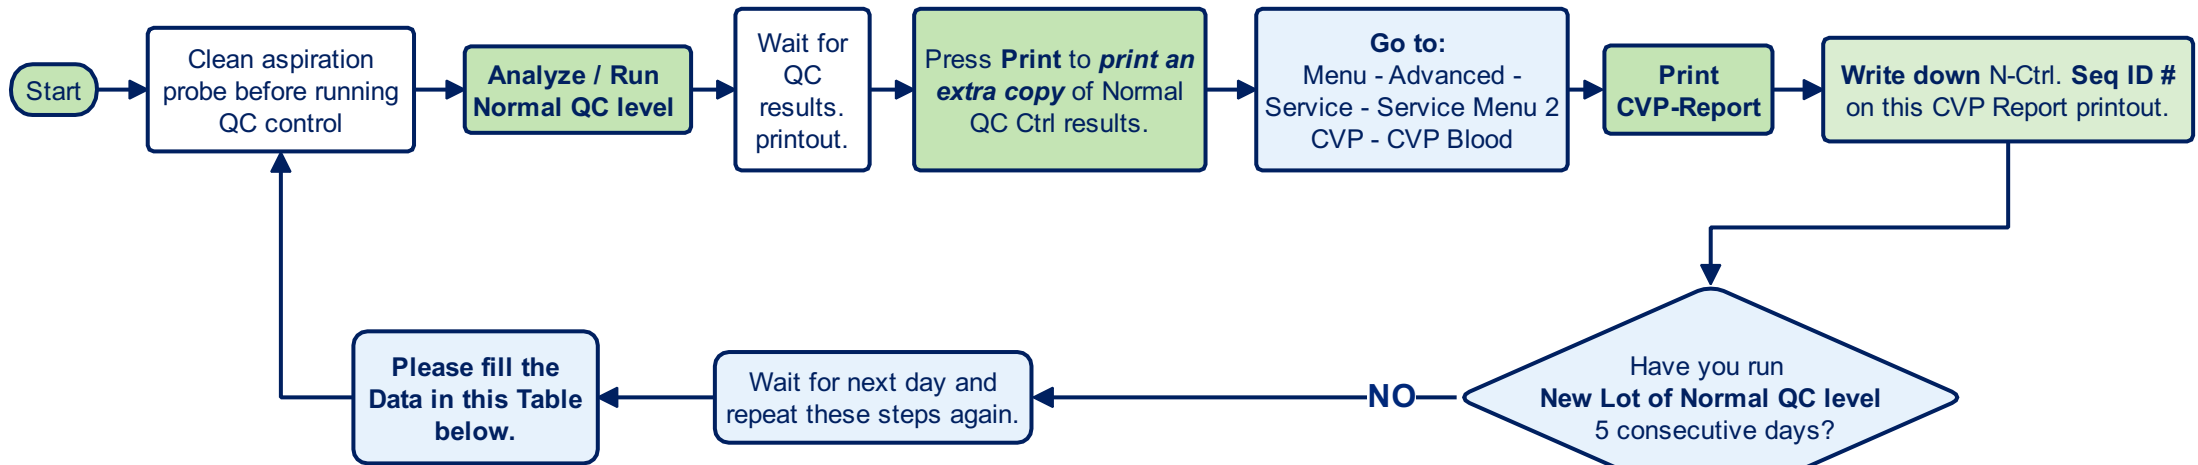

QC NORMAL CONTROL	RUN / DAY	SEQ ID#	RUN DATE	CVP-REPORT Grand Blood fl Value
LOT. NUMBER:	1			
	2			
EXP. DATE:	3			
	4			
	5			

Send this page as well as the Printouts in PDF format.
(5 ea. Normal Ctrl. & 5 ea. CVP Blood Reports)
to: CBCDiagnostics@gmail.com
Thank you.